



Saros Modular Chair

Assessment Form

1 Therapist and Users Details

Assessment Date:

Therapist Details

Name:

Organisation:

Email:

Telephone:

User Details

Name/Ref:

Address:

Email:

User Weight:

Pressure Care:

Posture:

Mobility:

Diagnosis:

Prognosis:

Transfer Method:

Current Seating:

Notes:



Information

If you require assistance in completing this form, please call our sales office on 01634 813388, or use our online chat facility at www.wealdenrehab.com/chat



2 Saros Chair Specifications

The Saros chair provides a comfortable chair on castors that is adaptable for different patient sizes and users that require pressure relief or additional support to sit with a good posture.

- Easily accessible push handles for carers
- Multi-adjustable pillow backrest as standard
- Integrated pressure care options
- Multi tilt range
- Multi back angle adjustments
- Arm height adjustment
- Adjustable seat width
- Multi seat ramp angle
- Webbed base seating system
- Footplate
- Four braked castors



Fabric Care

Wipe clean routinely with a microfibre cloth, lightly dampened with cold water only. Then dry with a clean absorbent cloth.

Soak up spillages as soon as possible with an absorbent dry cloth to prevent staining. Clean with a microfibre cloth, lightly dampened with cold water.

Note dyes and pigments from indigo jeans, ball point and felt tip pens may permanently stain.

If soiling has accumulated use a mild soap (non-alkaline). Take care to remove all soap residues. Then dry with an absorbent cloth.

Remove body fluids and extreme soiling immediately (within 15 minutes) with cold water. Apply your approved infection control protocol, a 10,000ppm sodium chlorite bleach solution, Haz-Tabs or Chlor-Clean. Remove product residues and then dry with a clean absorbent cloth.

Note steam cleaning disinfects but the application of heat may fix staining substances and may result in permanent marks.

Do not apply solvent based cleaners or any other chemicals to the fabric.


Do not dry clean, tumble dry or fully immerse the fabric in water.

3 Chair Configuration

Seat Width

1

Measure user's
hip to hip width

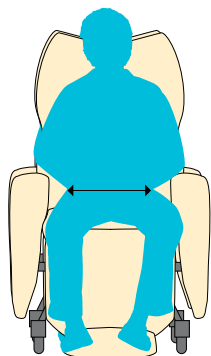


Choose closest seat width

- ☐ 405mm/16"
- ☐ 457mm/18"
- ☐ 508mm/20"

Seat Depth

2

Measure user's base
of spine to back of knee

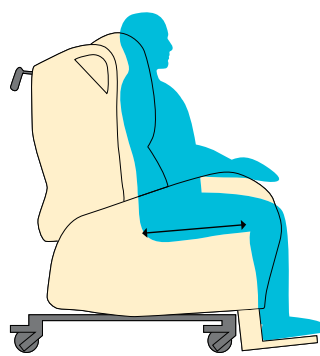


Choose closest seat depth

- ☐ 432mm/17"
- ☐ 457mm/18"
- ☐ 482mm/19"
- ☐ 508mm/20"
- ☐ 533mm/21"
- ☐ 559mm/22"

Seat Height

3

Measure user's
seat height

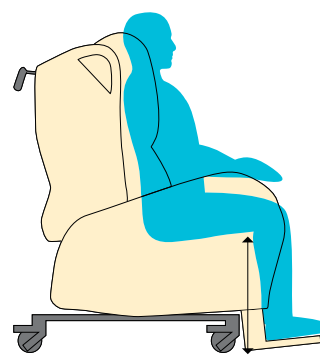

Choose seat height between
405-432mm / 16"-22"

4

Choose backrest angle



90°

STANDARD



100°



110°

5

Choose seat ramp angle



Flat

STANDARD



5°



10°

i Information

If the user's dimensions are outside of these parameters, please contact Wealden Rehab.

4 Pressure & Posture Management

Cushion choice

6

Visco-elastic cushion



Visco-elastic cushion – High risk pressure relieving cushion, to assist in prevention of pressure sores.



STANDARD

Integrated cushion



Cut-out allows integration of an alternating air cushion for users with existing pressure sores.



OPTIONAL

Backrest choice

7

Butterfly backrest



To provide extremely high levels of comfort, designed to accommodate patients with spinal curvature or in support where there may be muscle weakness.



STANDARD

Curved thoracic wedges



Pair of curved wedges to provide additional thoracic support, often of benefit for users with neurological conditions.



OPTIONAL

Thoracic backrest support



Thoracic backrest support – For users with kyphosis, offering a head cushion that protrudes further forward for support.



OPTIONAL

Headrest choice

8

Profiled horseshoe headrest



Fits over the shoulders for users with reduced head control.



OPTIONAL

5 Accessories

Additional Support

9

90° Footplate



90° fixed angle
padded footplate.



STANDARD

Angle Adjustable Footplate



Gives support to
feet and reduces risk
of foot drop. Vapour
permeable fabric.



OPTIONAL

Pelvic Strap



Safe, comfortable
positioning aid.



OPTIONAL

Four Point Pelvic Strap



Fixes to chair at four
points for additional
pelvic control for
safe, comfortable
positioning aid.



OPTIONAL

Actuation

10

Manual Operation



Fully manually
operated chair.



STANDARD

Electric Operation



Battery powered operation
of tilt-in-space and
legrest elevation allows
the user to adjust the
chair independently.




OPTIONAL


6 Dimensions Chart




Max Patient Weight
150kg / 23.5st

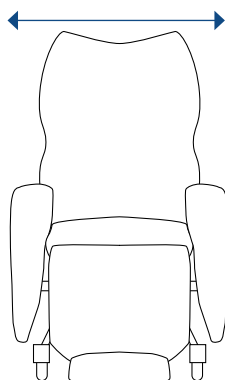


Overall Width
65-75cm / 26-30"

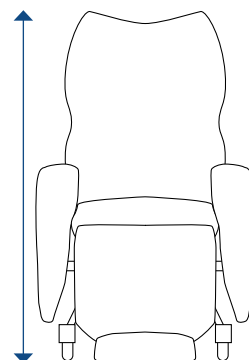


Overall Height
124cm / 49"

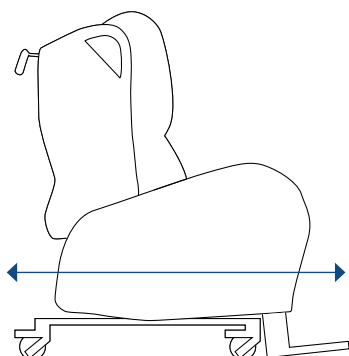


Overall Depth
105-127cm / 42-50"

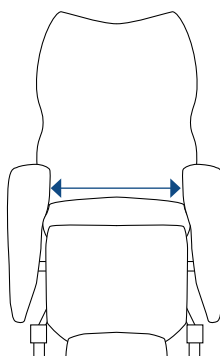


Seat Width
40-50cm / 16-20"

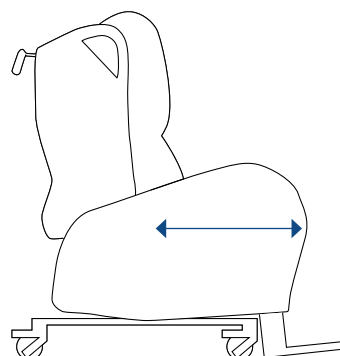


Seat Depth
40-55cm / 16-22"

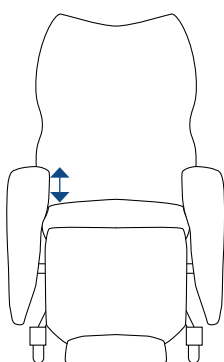

Arm Height
7", 8", 9"

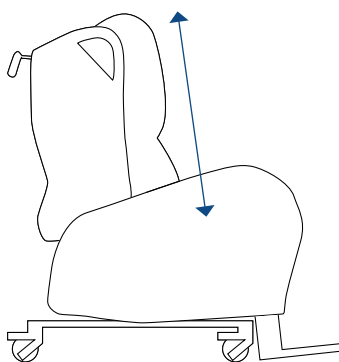

Back Height
76cm / 30"

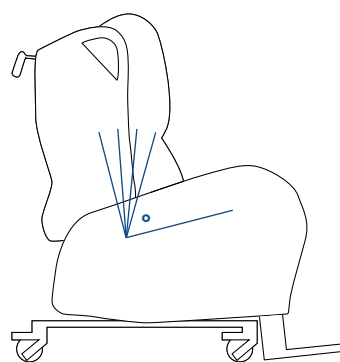

Back Angle
90, 80, 70, 60°

7