

# RAZ AP/SP Shower Chair

## Assessment Form



# 1 Therapist and Users Details

Assessment Date:

## Therapist Details

Name: .....

Organisation: .....

Email: .....

Telephone: .....

## User Details

Name/Ref: .....

Address: .....

.....

.....

Email: .....

User Weight: .....

Notes: .....

.....

.....

**i Information**  
If you require assistance in completing this form, please call our sales office on 01634 813388,  
or use our online chat facility at [www.wealdenrehab.com/chat](http://www.wealdenrehab.com/chat)




## 2 Chair Dimensions

### Seat Width

1


Measure user's  
hip to hip width:

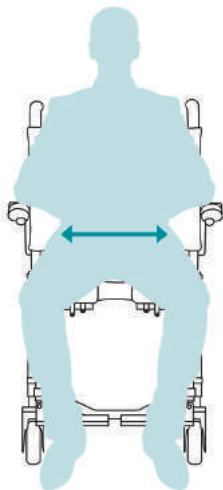

Fill in measurement:

2

Select which chair the user will fit into:

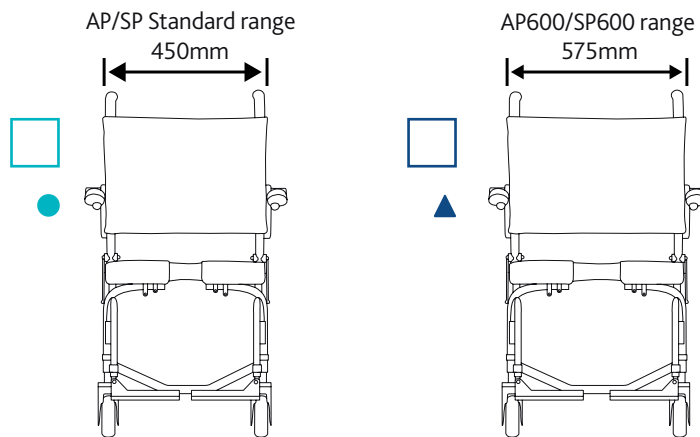

158kg AP/SP Standard Range	275kg AP600/SP600 Range
400mm - 520mm	520mm - 640mm

Select type of chair:

- ☐ Attendant Propelled (AP)
- ☐ Self Propelled (SP)

**Please note:** Custom made frames can be made to order up to 91cm (36") – Please call an adviser for details.

### **i** Information

If the user's dimensions are outside of this, please contact Wealden Rehab or your loan store.

When using a RAZ AP/SP over an automatic toilet you will need an special frame. Please call our sales office to discuss this further.

Examples of toilets that qualify as an automatic toilet;

- Clos-o-Mat
- Geberit Aquaclean 8000
- BioBidet




## 2 Chair Dimensions

### Seat Depth

3

Measure user's back to back of knee:

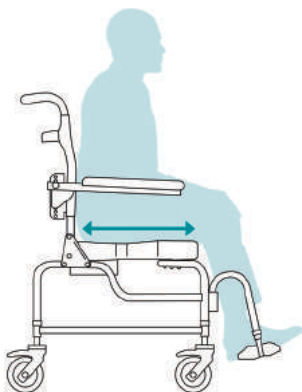







Fill in measurement:  
(Ideal chair depth)

#### **i** Information

Need extra pressure relief? See **page 7** for additional seat options.

3

Select which seat will best suit the user:

		<b>Bridged Seat</b> Bridged front design removes the risk of the users' leg falling into the gap of the seat – so consider this one for thinner users. Ideal for users with involuntary movement or those performing a side transfer.		<b>Open Front Seat</b> The open front seat gives the user and carer more access for personal hygiene. Opt for this seat when access is required and there is no risk of legs becoming entrapped in the gap.	
		<b>Length / Aperture Design</b>			
<b>158kg AP/SP Standard</b>	<b>400mm</b> Adjusts to accommodate 380 – 440mm seat depth	<input type="checkbox"/> ● <b>N0007</b>		<input type="checkbox"/> ● <b>N0006</b>	
	<b>475mm</b> Adjusts to accommodate 450 – 500mm seat depth	<input type="checkbox"/> ● <b>N0009</b>		<input type="checkbox"/> ● <b>N0008</b>	
<b>275kg AP600/SP600</b>	<b>450mm</b> Adjusts to accommodate 440 – 490mm seat depth			<input type="checkbox"/> ▲ <b>N0031</b>	



## 2 Chair Dimensions


### Seat Height

5

When choosing the seat height consider clearance required for the toilet, side transfer or standing transfer heights.

Please note: All dimensions assume the pan sliders are attached to the seat.

Removing the sliders will increase the dimension to the underside of seat by 25mm.

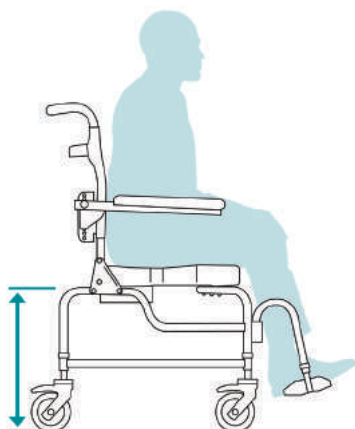

Toilet Bowl Height: (seat up)


Chair Seat Height:

Toilet bowl height (mm)	380	400	420	440	460	480	500	520
AP/SP Standard Seat Height	510	535	560	585	585	610	Please call an advisor	
AP600 5" Castor Seat Height	505	530	555	580	580	--		
AP600 6" Castor Seat Height	505	530	530	555	580	--		
SP600 5" Castor Seat Height	510	530	--	--	--	--		
SP600 6" Castor Seat Height	510	510	530	530	610	610	610	

### Arm Height

6

Specify arm height (default position is 248mm)

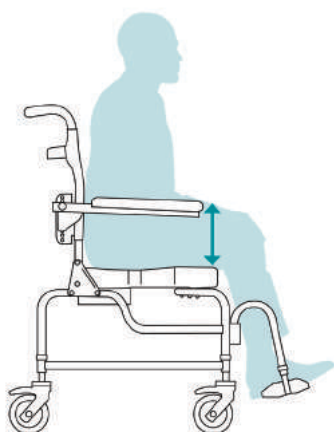


- ☐ 170mm
- ☐ 182mm
- ☐ 195mm
- ☐ 207mm
- ☐ 220mm
- ☐ 232mm
- ☐ 245mm

### Backrest Angle

7

Specify backrest angle (default position 90°)

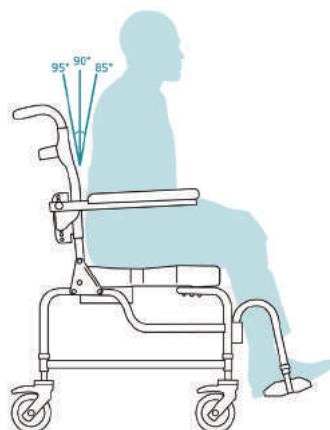


- ☐ 85°
- ☐ 90°
- ☐ 95°

## 2 Chair Dimensions

### Footplate Height

8

Measure user's lower leg length:

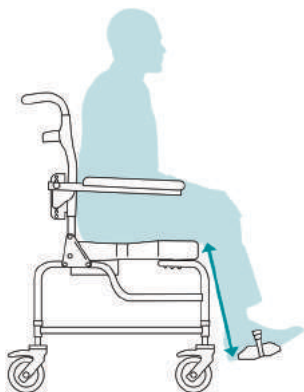

Seat to Footplate Dimension:  
(Standard 400-520mm)

#### Information

If the standard footplates are not suitable - see the accessories list of footplates on **page 6**.



# 3 Accessories

## Footplate Accessories\*

Suitable for: ● AP/SP Standard ▲ AP600/SP600



**N720** – Standard Footplates, pair, Adjustable 41-52cm, with folding plate.



**N2623** – Heavy Duty Footplates, pair, for RAZ Shower Chair. Adjustable 410-520mm, with folding plate. Heavy duty footplates for heavier users.



**N722** – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 300-410mm. For users with a lower leg length between 300-410mm.



**N721** – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 200-300mm. For users with a lower leg length between 200-300mm.



**N2628** – Neoprene Footplate Covers, for RAZ Standard Footplates. To give a softer texture under the users foot.



**N724** – Angle Adjustable Footplates for RAZ Rehab Shower Chair. Footplate can be angled to accommodate users with footdrop or if the ankle is in a fixed position.



**N729** – V-Style Footrest, with adjustable foot board and one-piece hangar, for RAZ Rehab Shower Chair. This footplate offers support for the feet in the centre of the chair. It cannot flip up or move out the way easily so normally used for hoisted patients.



**N2632** – Calf strap to give the legs support when the chair is tilted and to prevent feet from slipping backwards.



**N2822** – Flip-up one piece footplate. Flips back for transfers and reduces chair length for manoeuvrability. Adjusts in height 400mm – 510mm.

**N715/718/716/719** – The footplate elevates to support a leg that may be in extension. It also offers calf support. The options are for left and right and also for either a 400mm seat depth cushion or a 475mm seat depth.



**N715** – Elevating Legrest for RAZ Rehab Shower Chair to suit 450mm seat depth – Left side

**N718** – Right side



**N716** – Elevating Legrest for RAZ Rehab Shower Chair to suit 575mm seat depth – Left side

**N719** – Right side

\*Additional charge




## 3 Accessories



### Pressure Relief Seats\*

Suitable for: ● AP/SP Standard ▲ AP600/SP600

#### Visco Seat Options:

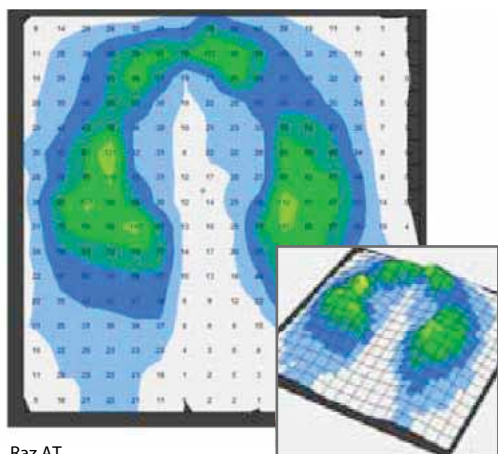

The Visco Seat option offers additional pressure relief for the user, and is recommended for those who suffer from pressure sores or are at high risk of acquiring one. These seats also give the option of side or rear access, which cannot be achieved with the standard range of seats.



Length / Aperture Design		Bridged Seat	Open Front Seat	Open Left Seat	Open Right Seat	Open Rear Seat
158kg AP/SP Standard Range	400mm Adjusts to accommodate 380 – 440mm seat depth	 N650	 N651	 N652	 N653	 N654
	475mm Adjusts to accommodate 450 – 500mm seat depth	 N655	 N656	 N657	 N658	 N659

#### **i** Information

If you are ordering the AP600/SP600 Shower chair, please call us on **01634 813388** for advice on Visco seats.

\*Additional charge



# 3 Accessories

## Postural Support Accessories\*

Suitable for: ● AP/SP Standard ▲ AP600/SP600



**N2676P** – Long PU pad for use with Leg Adductor Brackets – for RAZ-AT (Pair). This is provided to give side support on the chair. If a user is abducting, this will help their legs on the seat cushion.



**N690** – Swing-away Lateral Supports for RAZ Shower Chair, pair, complete with adjustable lateral pad and neoprene support wrap. These give thoracic support to the patient's torso, helping to keep their posture upright. They can be adjusted in height/depth and angle.



**N692** – Lateral Support Extension Plates for RAZ Rehab Shower Chair. This gives 25mm additional adjustment per side (50mm in total for a pair). These are used to reduce the width between the lateral support or the adductor pads.

Height from seat to top of lateral:

.....

Distance between laterals:

.....

## Headrest Support Accessories\*



**N731** – Standard headrest.



**C5960** – Head support cushion. This head cushion is flexible so can be curved around the users head. Comes with a stem to give height and depth adjustment.



**C5961** – Head support cushion. Very solid head support for clients who cannot support their own head. This support is not flexible.



**C5963** – Head support cushion. Most common headrest for users needing lateral support for their head. This is flexible so can wrap around the sides of the head to help support it in an upright position.



**N3906** – RAZ Headrest Clamp with 75mm Side-To-Side Offset Adjustment – specify this if the support required is not in the centreline of the chair.

No Image

\*Additional charge



# 3 Accessories

## Chair Accessories\*

Suitable for: ● AP/SP Standard ▲ AP600/SP600

### Backrest



**N2620** – Reclining AdjustaBack for RAZ Shower Chair, 500mm height, with adjustable flip-up armrests. Reclines to 30°.

### Arms



**N676** – Armrest Lock Kit for RAZ Rehab Shower Chair, pair. This kit stops the armrest moving up and therefore can be used for the patient to pull on and re-position. The lock releases to allow the arm to lift freely.



**N679** – Wide Soft Armpad for RAZ Rehab Shower Chair, 350mm x 80mm – Pair. This armrest offer a wider area of support for the patient's arms.



**N681** – These arm troughs help to keep the arm on the pad without falling off. There is angle and depth adjustment to the pads to suits the position of the users arms.



**N683** – Pivoting Arm Mount – Pair. These are used in conjunction with product codes N681 and N679, in order to allow the armpad to rotate through 90° and move into the upright position without conflicting with the backrest.

### Commode Pan



**N2581** – Commode Pan with handle and lid. Autoclavable.

\*Additional charge




## 4 Sizing Guide


### Dimension Chart – AP/SP




Max Patient Weight  
**158kg**

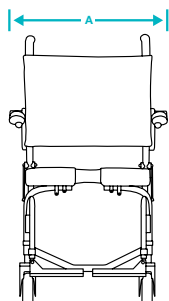


**A** Overall Width  
**575mm (AP)**  
**675mm (SP)**

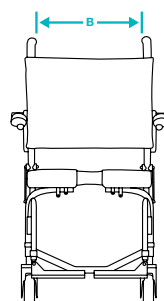


**B** Width between handles  
**400mm**




**C** Height from top of seat  
to top of backrest vinyl  
**420mm**




**D** Height from floor to  
top of push handles\*  
**1000mm**




**E** Top of seat from floor  
**510 / 535 / 560 /**  
**585 / 610mm**




**F** Underside of chassis  
side cross bar  
**200mm**




**G** Height of arm  
above seat  
**170 – 245mm**




**H** Depth of chassis  
**450mm**




**I** Overall depth  
without footrests  
**630mm (AP)**  
**760mm (SP)**




**J** Overall depth  
with footrests  
**870mm (AP)**  
**1000mm (SP)**




**K** Top of seat from  
standard footplates  
**410 – 520mm**



**L** Rearmost chair point to  
rear of seat aperture  
**260mm (AP)**  
**380mm (SP)**



**M** Front of chassis to  
front of footplates  
**250mm**



**N** maximum clearance for WC cistern\*  
**840 / 865 / 890 /**  
**915 / 940mm**

\*With 430mm standard backrest




## 4 Sizing Guide


### Dimension Chart – AP600/SP600




Max Patient Weight  
**275kg**

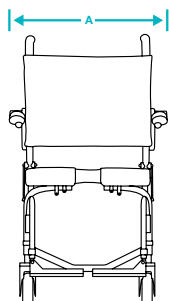


**A Overall Width**  
**670mm (AP600)**  
**770mm (SP600)**

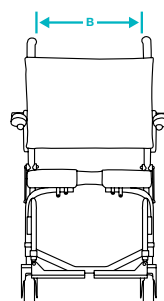


**B Width between handles**  
**500mm**




**C Height from top of seat to top of backrest vinyl**  
**520mm**




**D Height from floor to top of push handles\***  
**930mm**  
On lowest setting




**E Top of seat from floor**  
**490/510/540/570/600mm (AP600)**  
**510/530/610mm (SP600)**




**F Underside of chassis side cross bar**  
**200mm**




**G Height of arm above seat**  
**250mm**




**H Depth of chassis**  
**630mm**




**I Overall depth without footrests**  
**680mm (AP600)**  
**810mm (SP600)**




**J Overall depth with footrests**  
**930mm (AP600)**  
**1035mm (SP600)**




**K Top of seat from standard footplates**  
**410 – 520mm**



**L Rearmost chair point to rear of seat aperture**  
**255mm (AP600)**  
**380mm (SP600)**



**M Front of chassis to front of footplates**  
**250mm**



**N maximum clearance for WC cistern\***  
**780/805/830/855/880mm (AP600)**  
**805/825/905mm (SP600)**



## 5 Assessment Notes

