

RAZ AT Shower Chair Assessment Form



CELEBRATING
20
YEARS
2003-2023

1 Therapist and Users Details

Assessment Date:

Therapist Details

Name:

Organisation:

Email:

Telephone:

User Details

Name/Ref:

Address:

.....

.....

Email:

User Weight:

Notes:

.....

.....

Information

If you require assistance in completing this form, please call our sales office on 01634 813388, or use our online chat facility at www.wealdenrehab.com/chat



2 Core Stock Chair

Core Stock Chair includes:

RAZ AT N0001 Frame

plus



N2581

Open Front Seat
18x16



N676

Standard Armrests



N2632

Calf strap



N731

Standard Headrest



N2581

Commode pan

Ordering details to include:

- **Seat Height**
- **Armrest Height**
- **Backrest Angle**



Information

Seat measurements can be configured on **pages 6 & 7**.

Set Up:

On delivery the prescriber is required to adjust:

- **Tension Adjustable Backrest**
- **Pelvic alignment**
- **Footplate Height**




2 Chair Dimensions

Seat Width

1

Measure the outside
of the users pelvis:

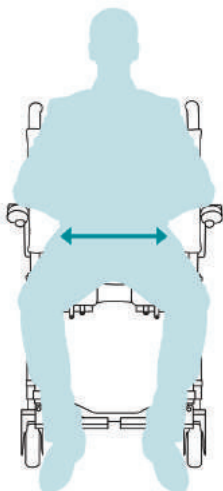


Fill in measurement:

2

AT Standard range

450mm

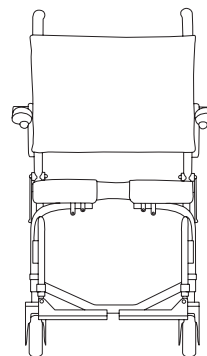

185kg
AT Standard Range

accommodates a hip width of
400mm - 520mm



CORE STOCK ITEM

Arm Height

3

Specify arm height (default position is 248mm)

	L		R
	<input type="checkbox"/>	200mm	<input type="checkbox"/>
	<input type="checkbox"/>	212mm	<input type="checkbox"/>
	<input type="checkbox"/>	224mm	<input type="checkbox"/>
	<input type="checkbox"/>	236mm	<input type="checkbox"/>
	<input type="checkbox"/>	248mm	<input type="checkbox"/>
	<input type="checkbox"/>	260mm	<input type="checkbox"/>
	<input type="checkbox"/>	272mm	<input type="checkbox"/>

4

Specify backrest angle (default position 90°)

	<input type="checkbox"/>	90°
	<input type="checkbox"/>	95°




2 Chair Dimensions

Seat Depth

5

Measure user's back to back of knee:

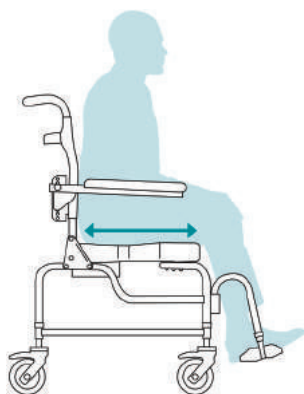

Fill in measurement:
(Ideal chair depth)







Information

Need extra pressure relief? See **page 9** for additional seat options.

6

Select which seat will best suit the user:

		Bridged Seat		Open Front Seat	
		Bridged front design removes the risk of the users' leg falling into the gap of the seat – so consider this one for thinner users. Ideal for users with involuntary movement or those performing a side transfer.		The open front seat gives the user and carer more access for personal hygiene. Opt for this seat when access is required and there is no risk of legs becoming entrapped in the gap.	
185kg AT Standard	Length / Aperture Design				
	400m Adjusts to accommodate 380 – 440mm seat depth	<input type="checkbox"/>		<input checked="" type="checkbox"/>	
		N0007		CORE STOCK ITEM N0006	
185kg AT Standard	475mm Adjusts to accommodate 450 – 500mm seat depth	<input type="checkbox"/>		<input type="checkbox"/>	
		N0009		N0008	




2 Chair Dimensions

Seat Height

7

When choosing the seat height consider clearance required for the toilet, side transfer or standing transfer heights.

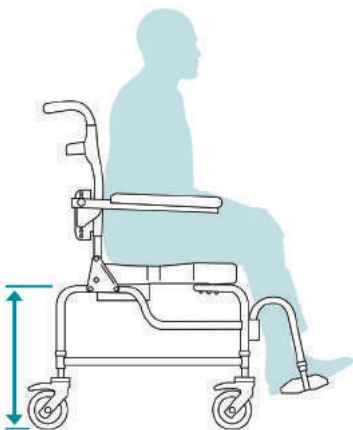

Toilet Bowl Height: (seat up)

.....

Chair Seat Height:


.....

Toilet bowl height (mm)	380	400	420	440	460	480	500	520
AT Standard Seat Height	530	530	560	560	580	610	640	640



2 Chair Dimensions

Lining up your chair with the toilet bowl

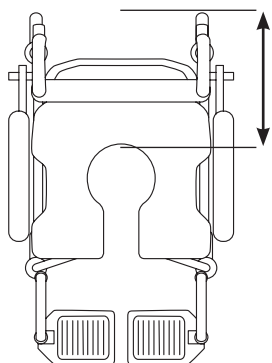

Rearmost chair point
to rear of seat aperture

AP = 180mm

ART = 265mm

SP = 280mm

AT = 340mm

Using an automatic WC?

Geberit:

All RAZ chairs are compatible with the Geberit Mera Care toilet.

For the Geberit 7000 and Aquaclean 8000, the RAZ ATW, RAZ ART and AP Auto provide the best fit.

Closomat:

For a tilt in space chair, the RAZ ATW and RAZ-ART fit well over the Closomat toilet.

For an attendant and self-propel option, we suggest using the RAZ-AP Auto, this can also be upgraded with a self-propel wheel kit.

Bio-Bidet:

RAZ chairs are not compatible with the BioBidet.


Best practice

A common requirement is to have the skirt accessory added to the underside of the seat and the option of removing the pan sliders to provide a closer fit with the toilet. The standard moulded seat shaping contributes to a much improved wash experience.

Footplate Height

8

Measure user's lower leg length:

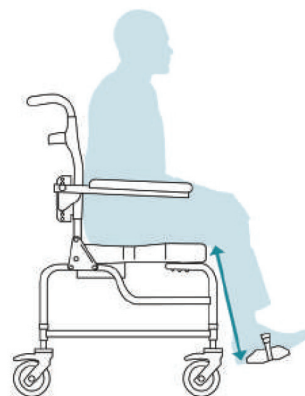

Seat to Footplate Dimension:

(Standard 400-520mm)

i Information

If the standard footplates are not suitable - see the accessories list of footplates on **page 8**.



3 Accessories – Additional Cost

Footplate Accessories*



N720 – Standard Footplates, pair, Adjustable 41-52cm, with folding plate.

CORE STOCK ITEM



N2632 – Calf strap to give the legs support when the chair is tilted and to prevent feet from slipping backwards.

CORE STOCK ITEM



N2628 – Neoprene Footplate Covers, for RAZ Standard Footplates. To give a softer texture under the users foot.



N721 – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 200-300mm. For users with a lower leg length between 200-300mm.



N722 – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 300-410mm. For users with a lower leg length between 300-410mm.




N724 – Angle Adjustable Footplates for RAZ Rehab Shower Chair. Footplate can be angled to accommodate users with footdrop or if the ankle is in a fixed position.



N729 – V-Style Footrest, with adjustable foot board and one-piece hangar, for RAZ Rehab Shower Chair. This footplate offers support for the feet in the centre of the chair. It cannot flip up or move out the way easily so normally used for hoisted patients.



N2632 – Bodypoint Aeromesh Calf Strap.

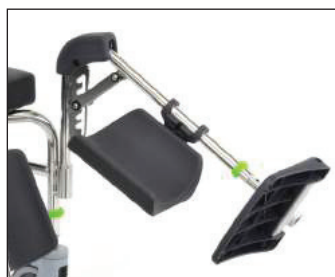

N715 – Elevating Legrest for RAZ Rehab Shower Chair to suit 450mm seat depth – Left side



N716 – Elevating Legrest for RAZ Rehab Shower Chair to suit 575mm seat depth – Left side



N718 – Right side



N719 – Right side

N715/718/716/719 – The footplate elevates to support a leg that may be in extension. It also offers calf support. The options are for left and right and also for either a 400mm seat depth cushion or a 475mm seat depth.


*Additional charge





3 Accessories – Additional Cost

Pressure Relief Seats*

Visco Seat Options:

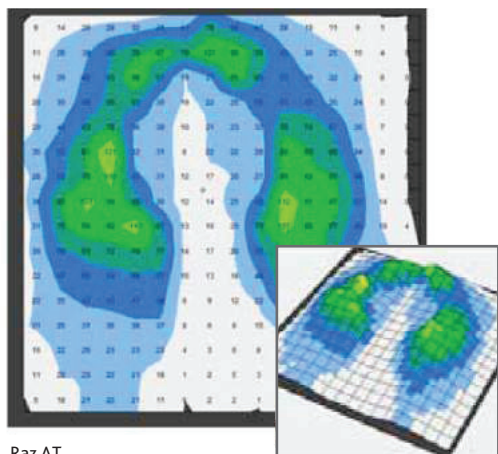

The Visco Seat option offers additional pressure relief for the user, and is recommended for those who suffer from pressure sores or are at high risk of acquiring one. These seats also give the option of side or rear access, which cannot be achieved with the standard range of seats.



Length / Aperture Design		Bridged Seat	Open Front Seat	Open Left Seat	Open Right Seat	Open Rear Seat
136kg AT Standard Range	400mm Adjusts to accommodate 380 – 440mm seat depth	<input type="checkbox"/> N650	<input type="checkbox"/> N651	<input type="checkbox"/> N652	<input type="checkbox"/> N653	<input type="checkbox"/> N654
	475mm Adjusts to accommodate 450 – 500mm seat depth	<input type="checkbox"/> N655	<input type="checkbox"/> N656	<input type="checkbox"/> N657	<input type="checkbox"/> N658	<input type="checkbox"/> N659
		<input type="checkbox"/> No Pressure Relief Seat				

i Information




If you are ordering the AT600 Shower chair, please call us on **01634 813388** for advice on Visco seats.

*Additional charge



3 Accessories – Additional Cost

Postural Support Accessories*

<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>N2676P – Long PU pad for use with Leg Adductor Brackets – for RAZ-AT (Pair). This is provided to give side support on the chair. If a user is abducting, this will help their legs on the seat cushion.</p> </div> </div>	<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>N690 – Swing-away Lateral Supports for RAZ Shower Chair, pair, complete with adjustable lateral pad and neoprene support wrap. These give thoracic support to the patient's torso, helping to keep their posture upright. They can be adjusted in height/depth and angle.</p> </div> </div>
<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>N692 – Lateral Support Extension Plates for RAZ Rehab Shower Chair. This gives 25mm additional adjustment per side (50mm in total for a pair). These are used to reduce the width between the lateral support or the adductor pads.</p> </div> </div>	<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p>Height from seat to top of lateral:</p> <p>.....</p> </div> <div style="width: 45%;"> <p>Distance between laterals:</p> <p>.....</p> </div> </div>

Headrest Support Accessories*

<div style="display: flex; align-items: flex-start;"> <input checked="" type="checkbox"/> <div style="margin-left: 10px;">  <p>N731 – Standard headrest. CORE STOCK ITEM</p> </div> </div>	<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>C5960 – Head support cushion. This head cushion is flexible so can be curved around the users head. Comes with a stem to give height and depth adjustment.</p> </div> </div>
<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>C5961 – Head support cushion. Very solid head support for clients who cannot support their own head. This support is not flexible.</p> </div> </div>	<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>C5963 – Head support cushion. Most common headrest for users needing lateral support for their head. This is flexible so can wrap around the sides of the head to help support it in an upright position.</p> </div> </div>
<div style="display: flex; align-items: flex-start;"> <input type="checkbox"/> <div style="margin-left: 10px;">  <p>N3906 – RAZ Headrest Clamp with 75mm Side-To-Side Offset Adjustment – specify this if the support required is not in the centreline of the chair.</p> </div> </div>	

*Additional charge

3 Accessories – Additional Cost

Chair Accessories*

Backrest



N2620 – Reclining AdjustaBack for RAZ Shower Chair, 500mm height, with adjustable flip-up armrests. Reclines to 30°. NB Chassis Tilt will be limited to 25°.

Arms



N676 – Standard Armrests Flip-up for easy access and transfers (come as part of Adjustaback)

CORE STOCK ITEM



N676 – Armrest Lock Kit for RAZ Rehab Shower Chair, pair. This kit stops the armrest moving up and therefore can be used for the patient to pull on and re-position. The lock releases to allow the arm to lift freely.



N681 – These arm troughs help to keep the arm on the pad without falling off. There is angle and depth adjustment to the pads to suits the position of the users arms.



N679 – Wide Soft Armpad for RAZ Rehab Shower Chair, 350mm x 80mm – Pair. This armrest offer a wider area of support for the patient's arms.



N683 – Pivoting Arm Mount – Pair. These are used in conjunction with product codes N681 and N679, in order to allow the armpad to rotate through 90° and move into the upright position without conflicting with the backrest.

Self Propelling Wheels



N3157 – Self propel kit for AT. A kit to change an attendant tilt chair to a self propelled tilt chair. This kit fits to any standard RAZ-AT and includes anti-tips and brake levers. Wheels with textured push rim.

Commode Pan



N2581 – Commode Pan with handle and lid. Autoclavable.

CORE STOCK ITEM

Chest Harness



Flex-Contol harnesses offer a greater range of posture



5.71032 – Mens



5.71034 – Womens

Shower Hip Belt



3001 - S



3002 - M



3003 - L

*Additional charge




4 Sizing Guide


Dimension Chart – AT




Max Patient Weight
185kg




A Overall Width
605mm




B Width between handles
400mm




C Height from top of seat
to top of backrest vinyl
520mm




D Height from floor to
top of push handles*
1000mm




E Top of seat from floor
**530 / 560 / 580 /
610 / 640mm**




F Underside of chassis
side cross bar
180mm




G Height of arm
above seat
200 – 260mm




H Depth of chassis
450mm




I Overall depth
without footrests
740mm




J Overall depth
with footrests
980mm




K Top of seat from
standard footplates
410 – 520mm




L Rearmost chair point to
rear of seat aperture
330mm



M Front of chassis to
front of footplates
250mm



N overall depth with
footplates, in full tilt
1300mm



O maximum clearance for WC cistern*
**920 / 950 / 980 /
1010 / 1040mm**



5

